

Processing Record for this file:
(Make notes here unique for this file)

Loading 5/1 - 6/1/2014
Data loaded directly from DMF


Processed CO data normally.
Ambient CO data appear normal and acceptable.

Standard additions show minimal variation over the month


2014-04-17 06:00 - 2014-05-09 06:00 Calibration cylinder was either turned off or expired.

For whatever reason, instrument responded without incident this month. No evidence of temperature sensor problems.


Los Gatos Model ICOS CO/N2O/H2O Analyzer

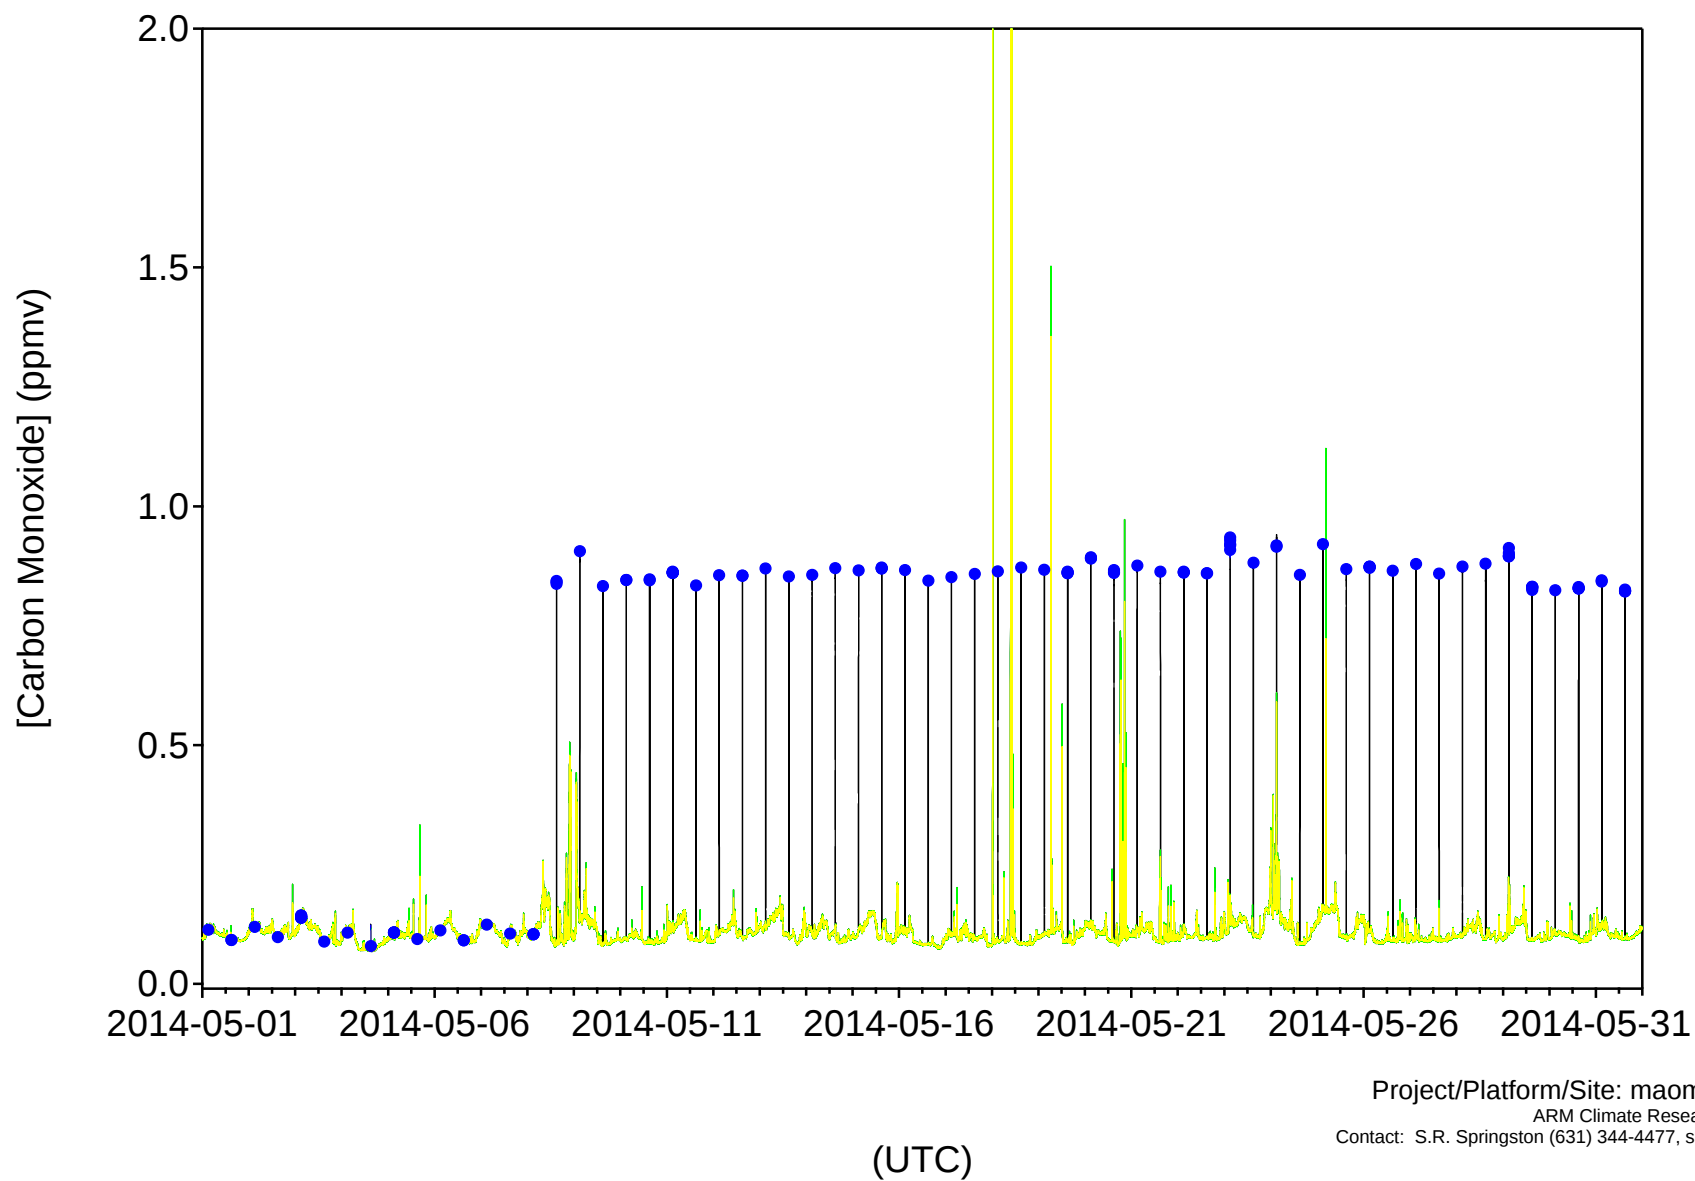


Los Gatos Model ICOS CO/N2O/H2O Analyzer
Housekeeping

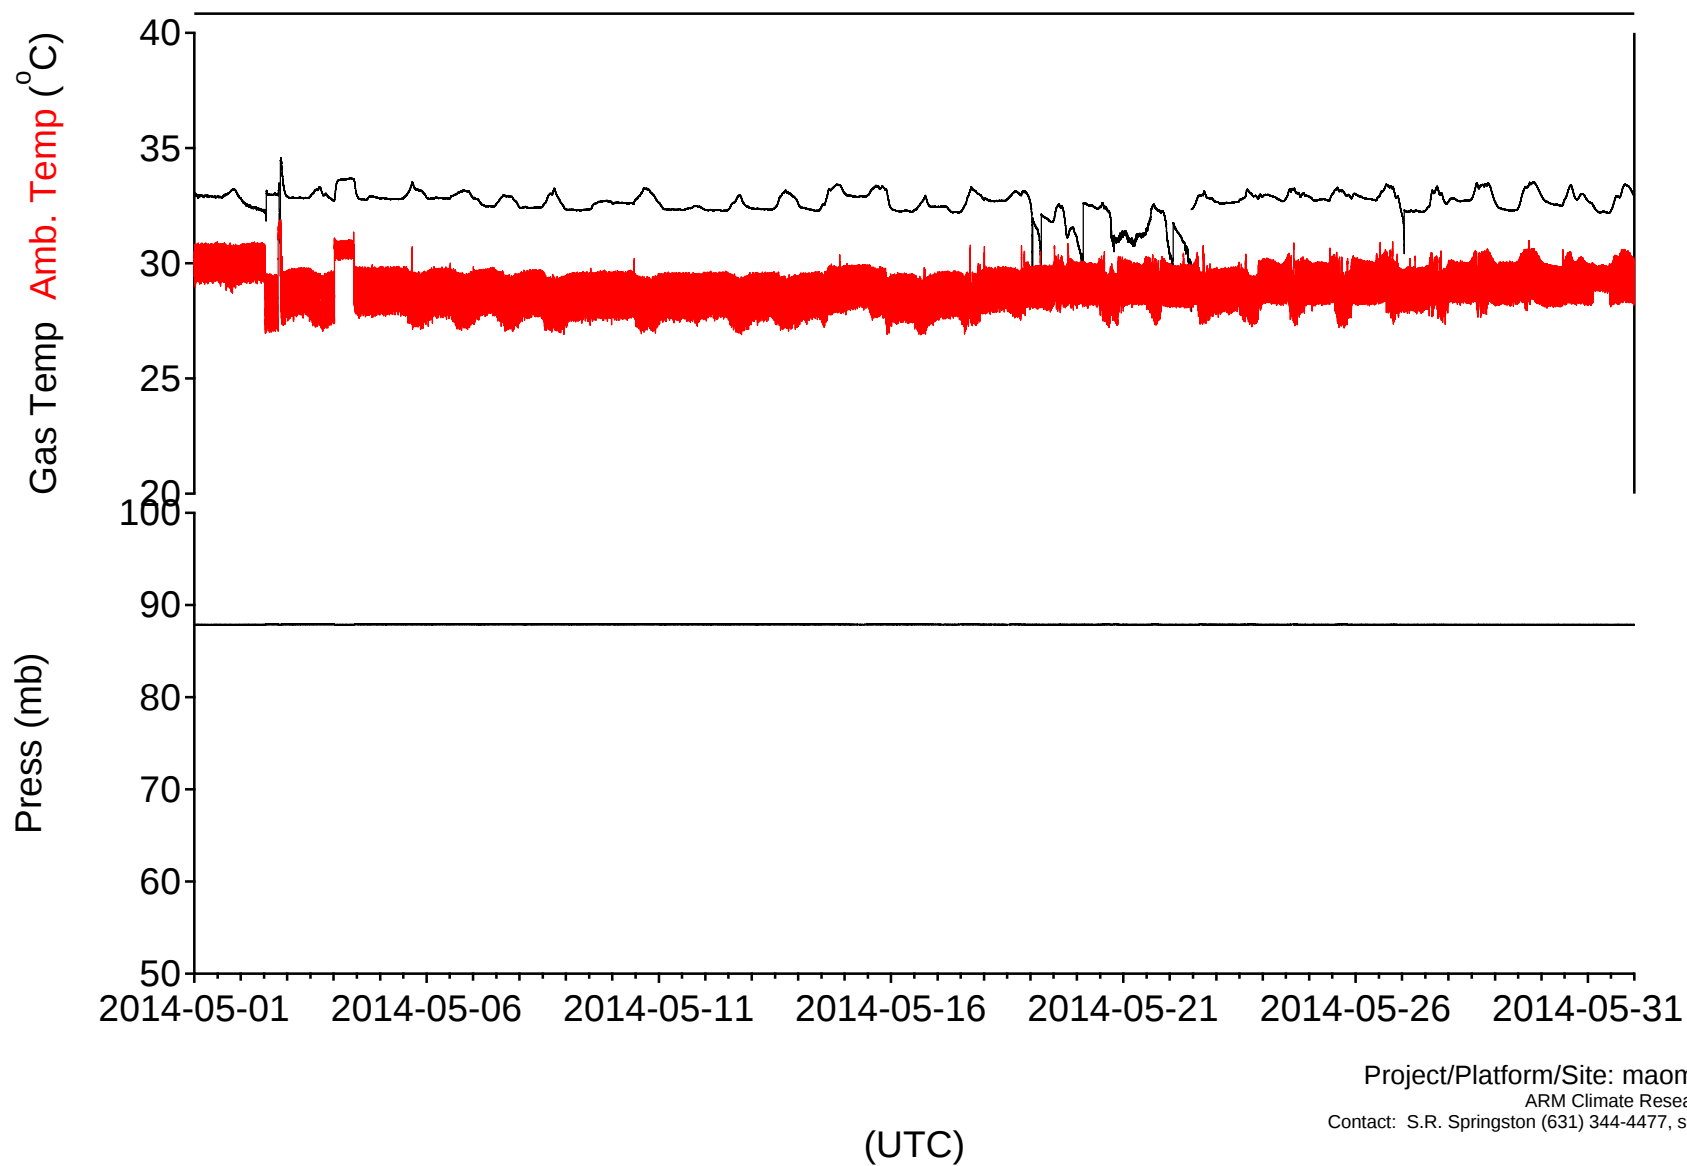


Los Gatos Model ICOS CO/N2O/H2O Analyzer Span Checks

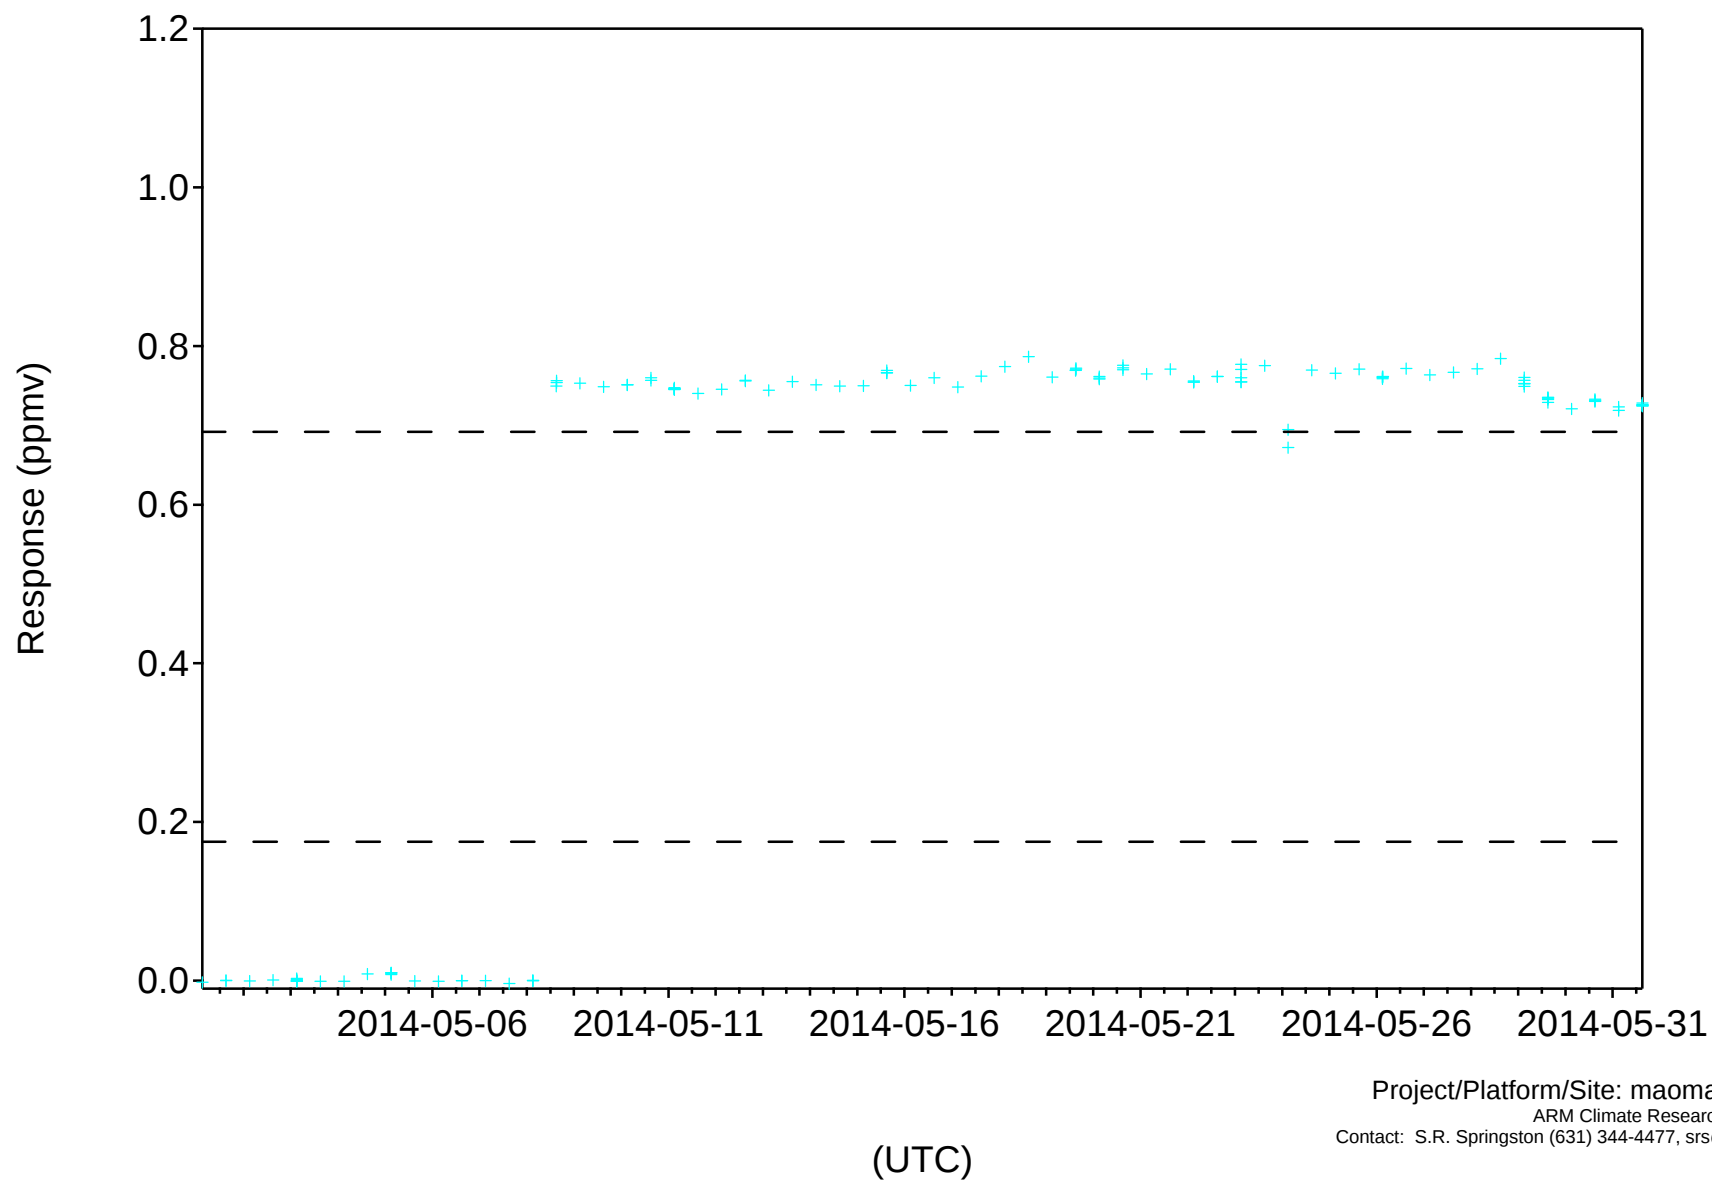

Los Gatos Model ICOS CO/N2O/H2O Analyzer

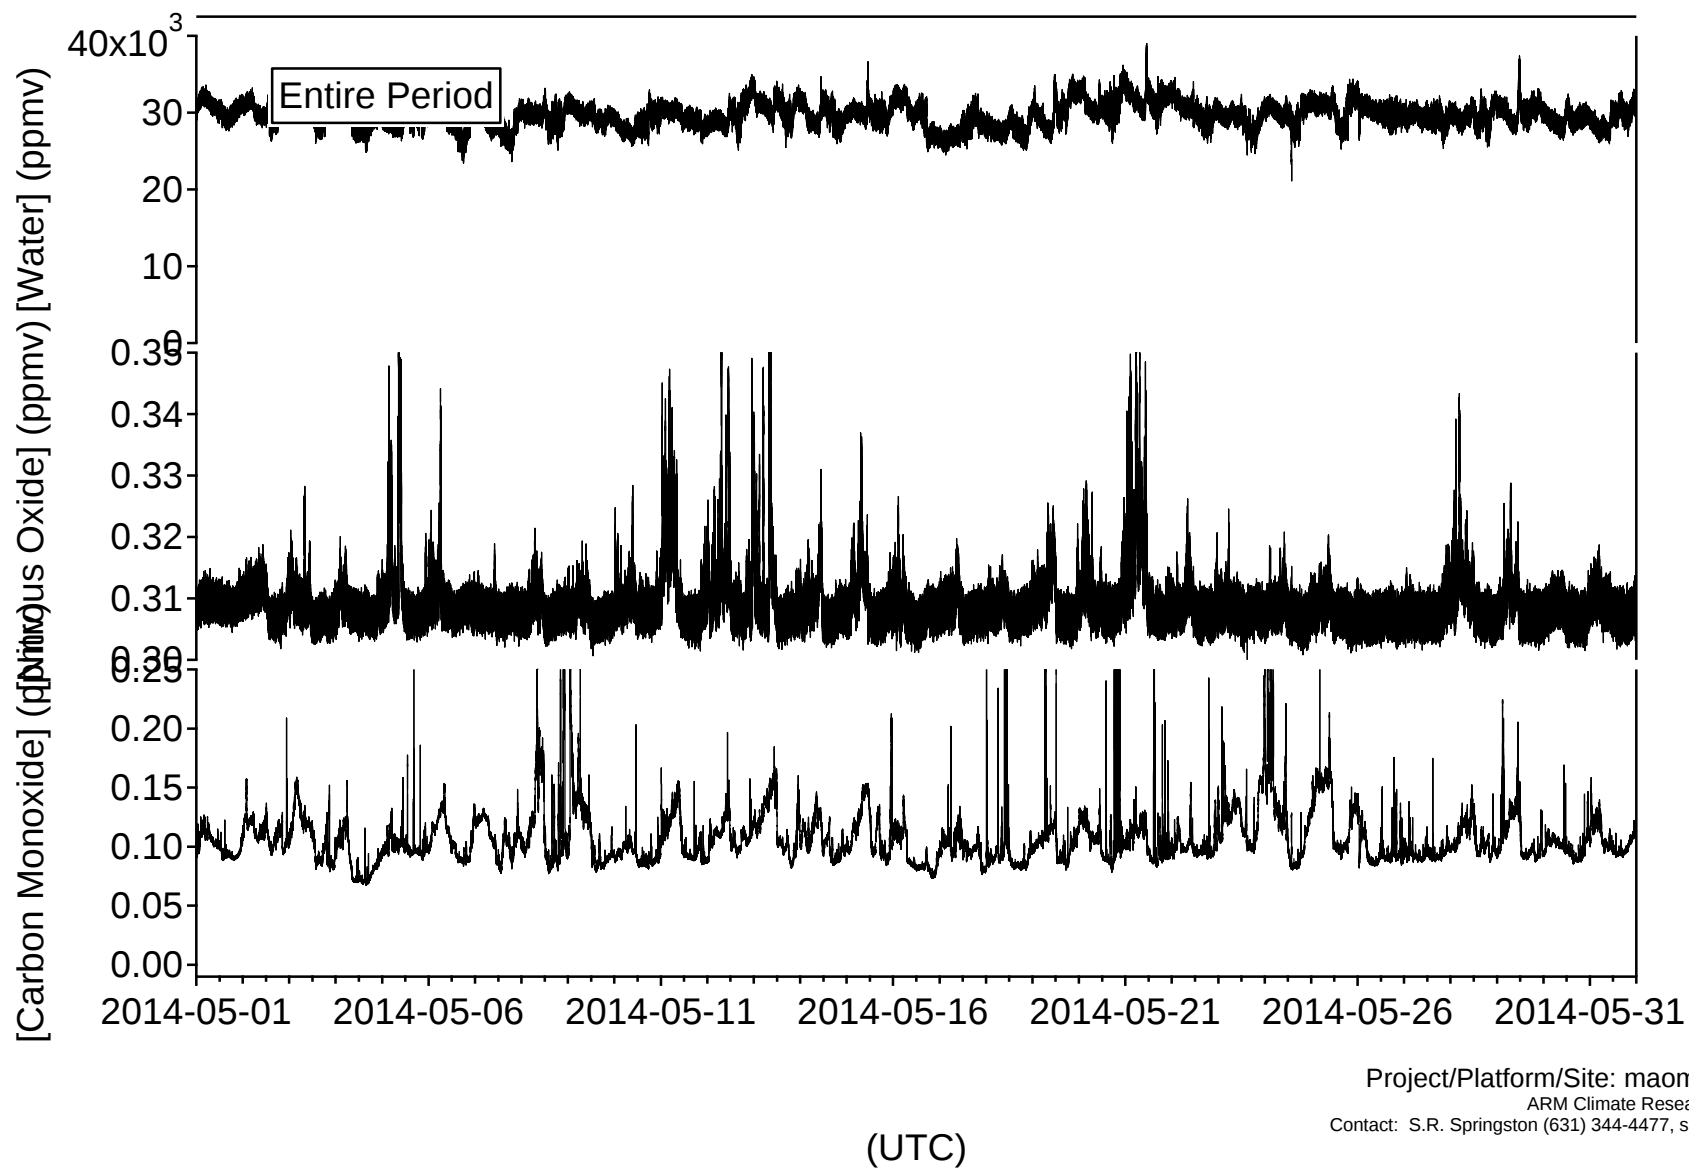


Los Gatos Model ICOS CO/N2O/H2O Analyzer

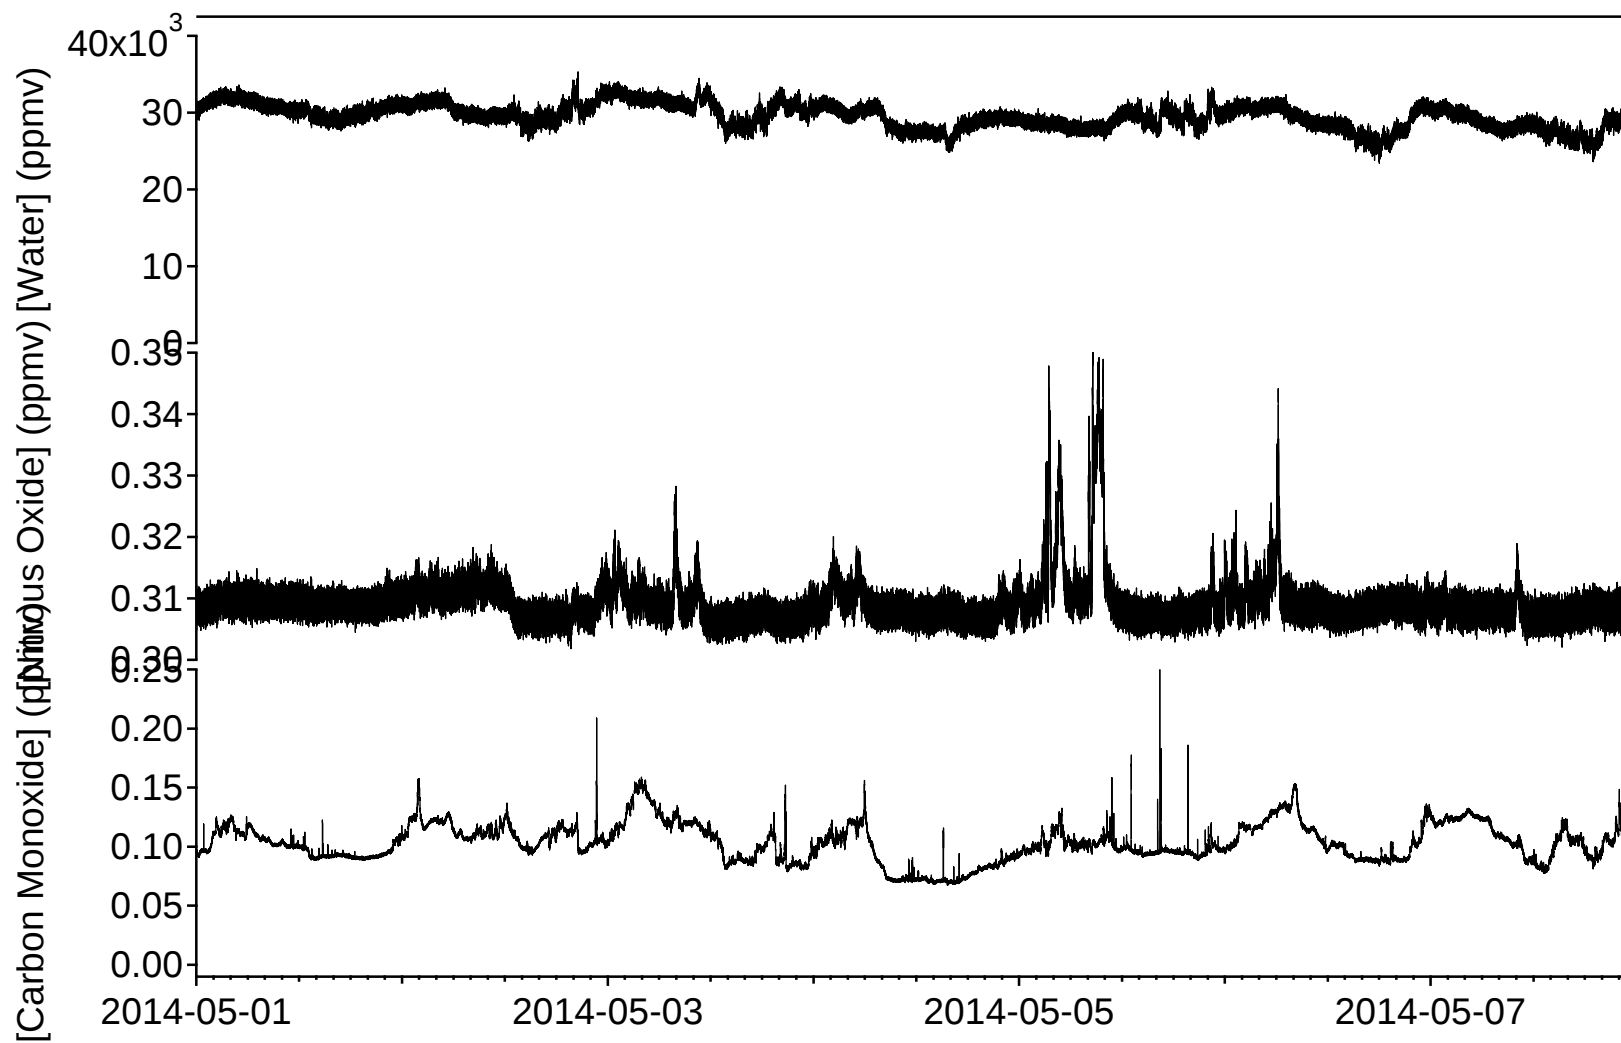


(UTC)

Project/Platform/Site: maomaoscs1
ARM Climate Research Facility
Contact: S.R. Springston (631) 344-4477, srs@bnl.gov

Los Gatos Model ICOS CO/N2O/H2O Analyzer

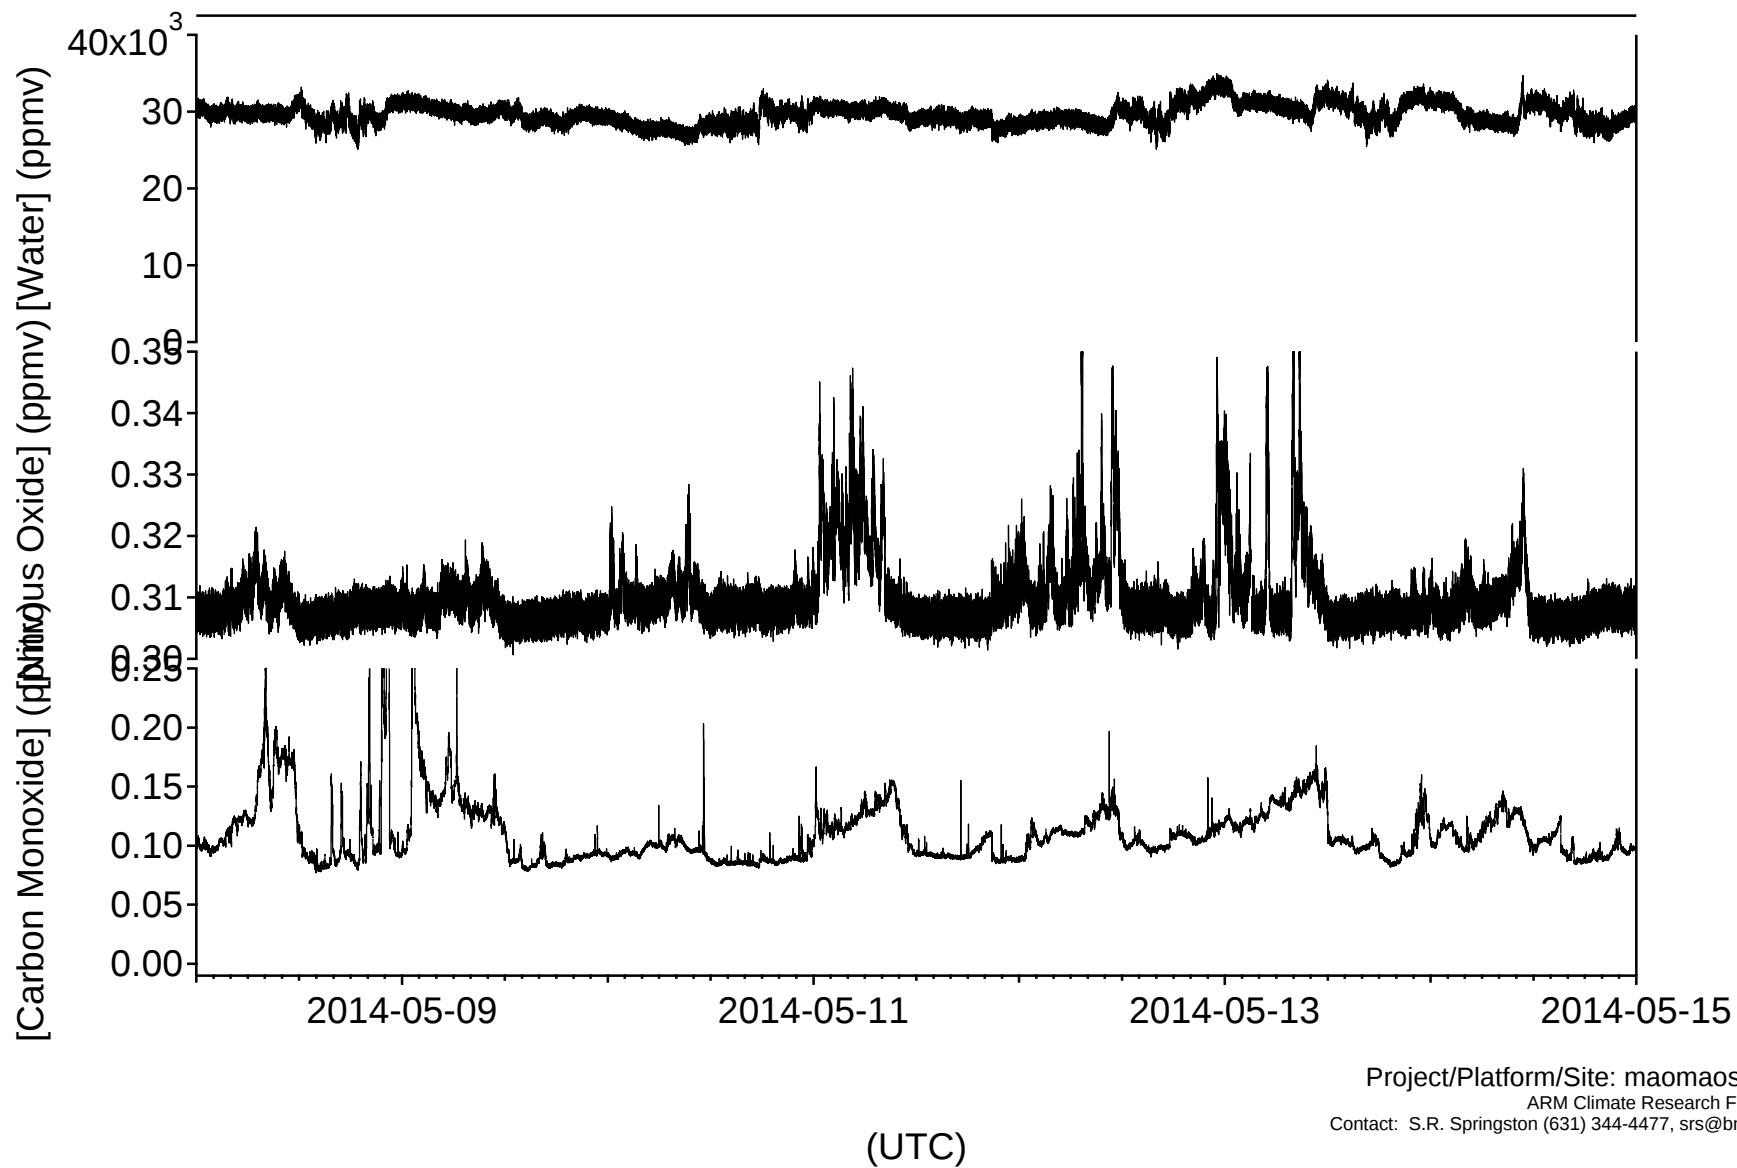


Los Gatos Model ICOS CO/N2O/H2O Analyzer

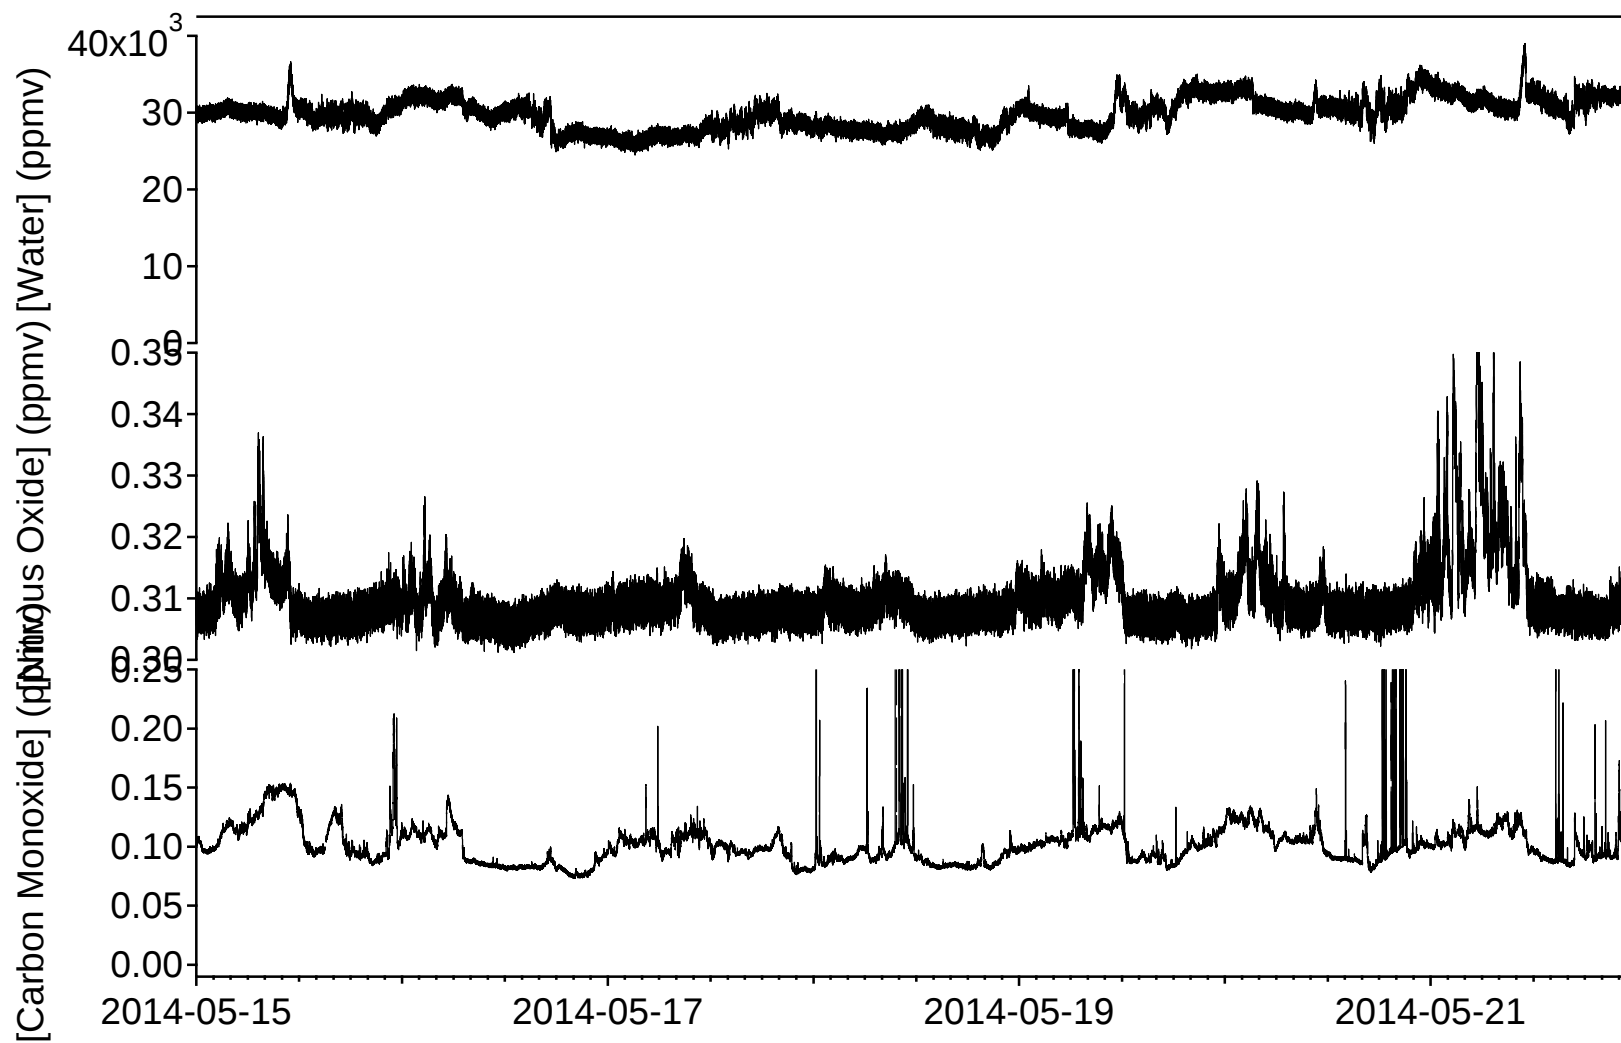

(UTC)

Project/Platform/Site: maomaoscs1
ARM Climate Research Facility
Contact: S.R. Springston (631) 344-4477, srs@bnl.gov


Los Gatos Model ICOS CO/N2O/H2O Analyzer

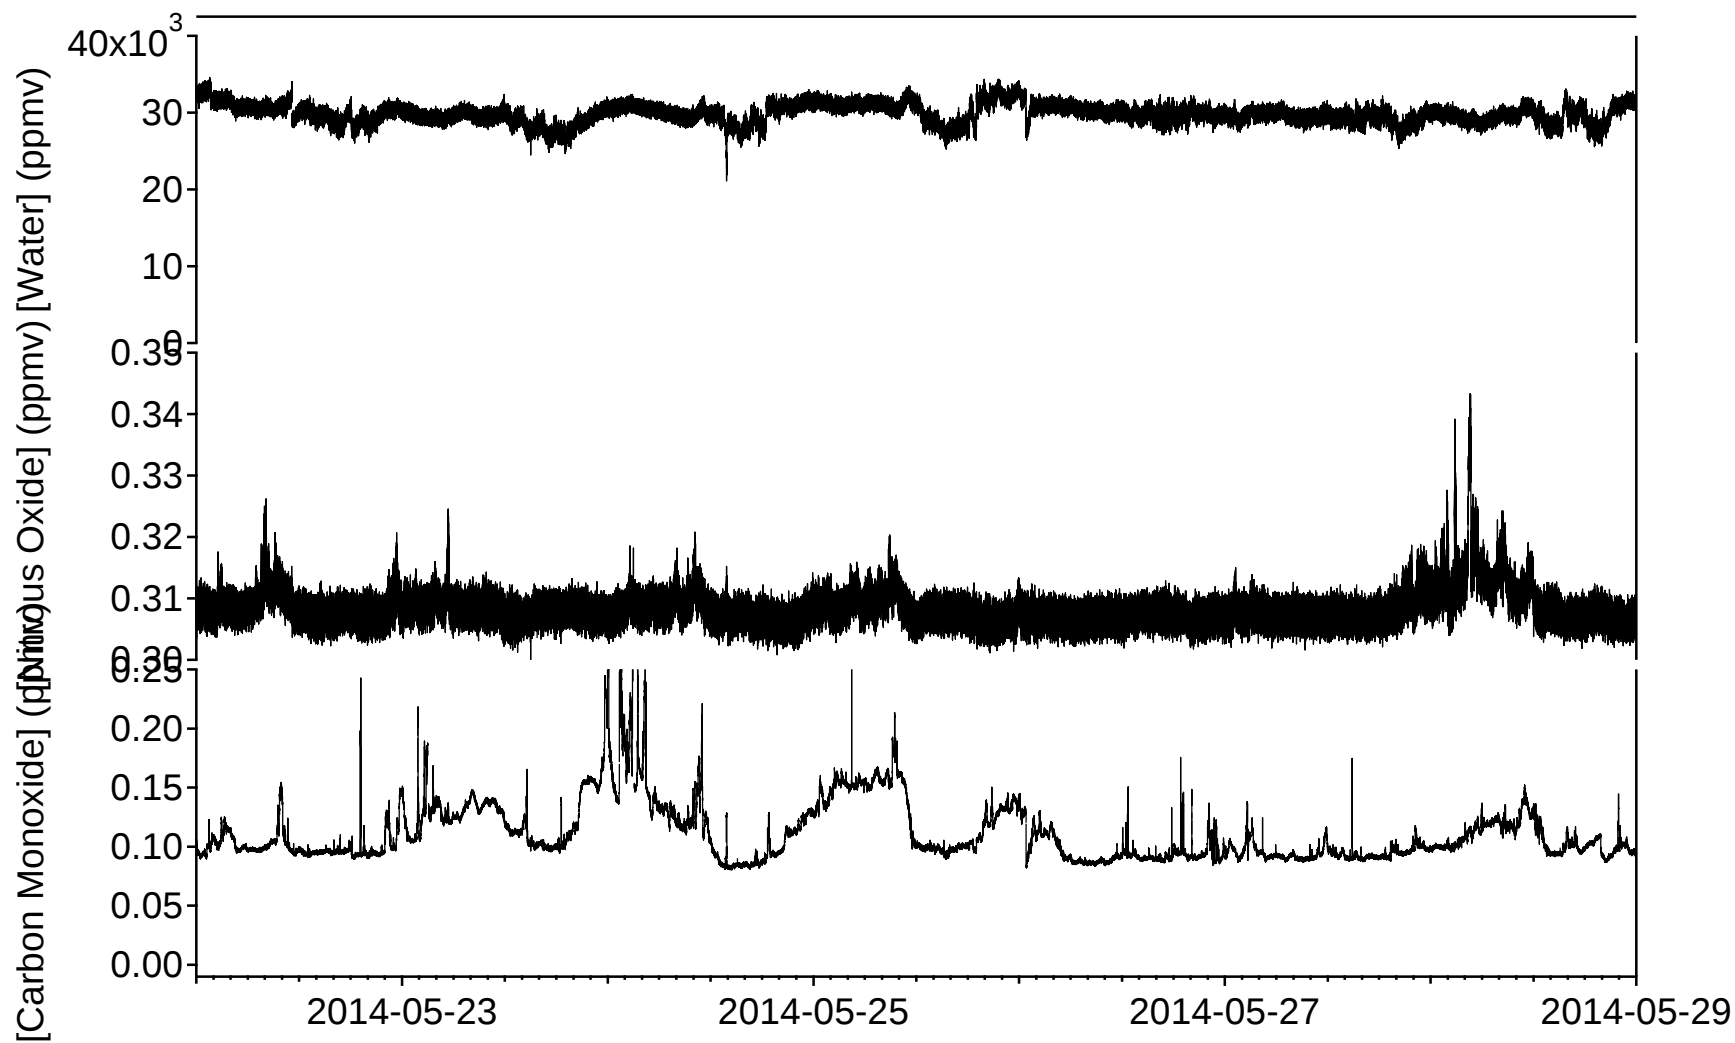

(UTC)

Project/Platform/Site: maomaoscs1
ARM Climate Research Facility
Contact: S.R. Springston (631) 344-4477, srs@bnl.gov

Los Gatos Model ICOS CO/N2O/H2O Analyzer

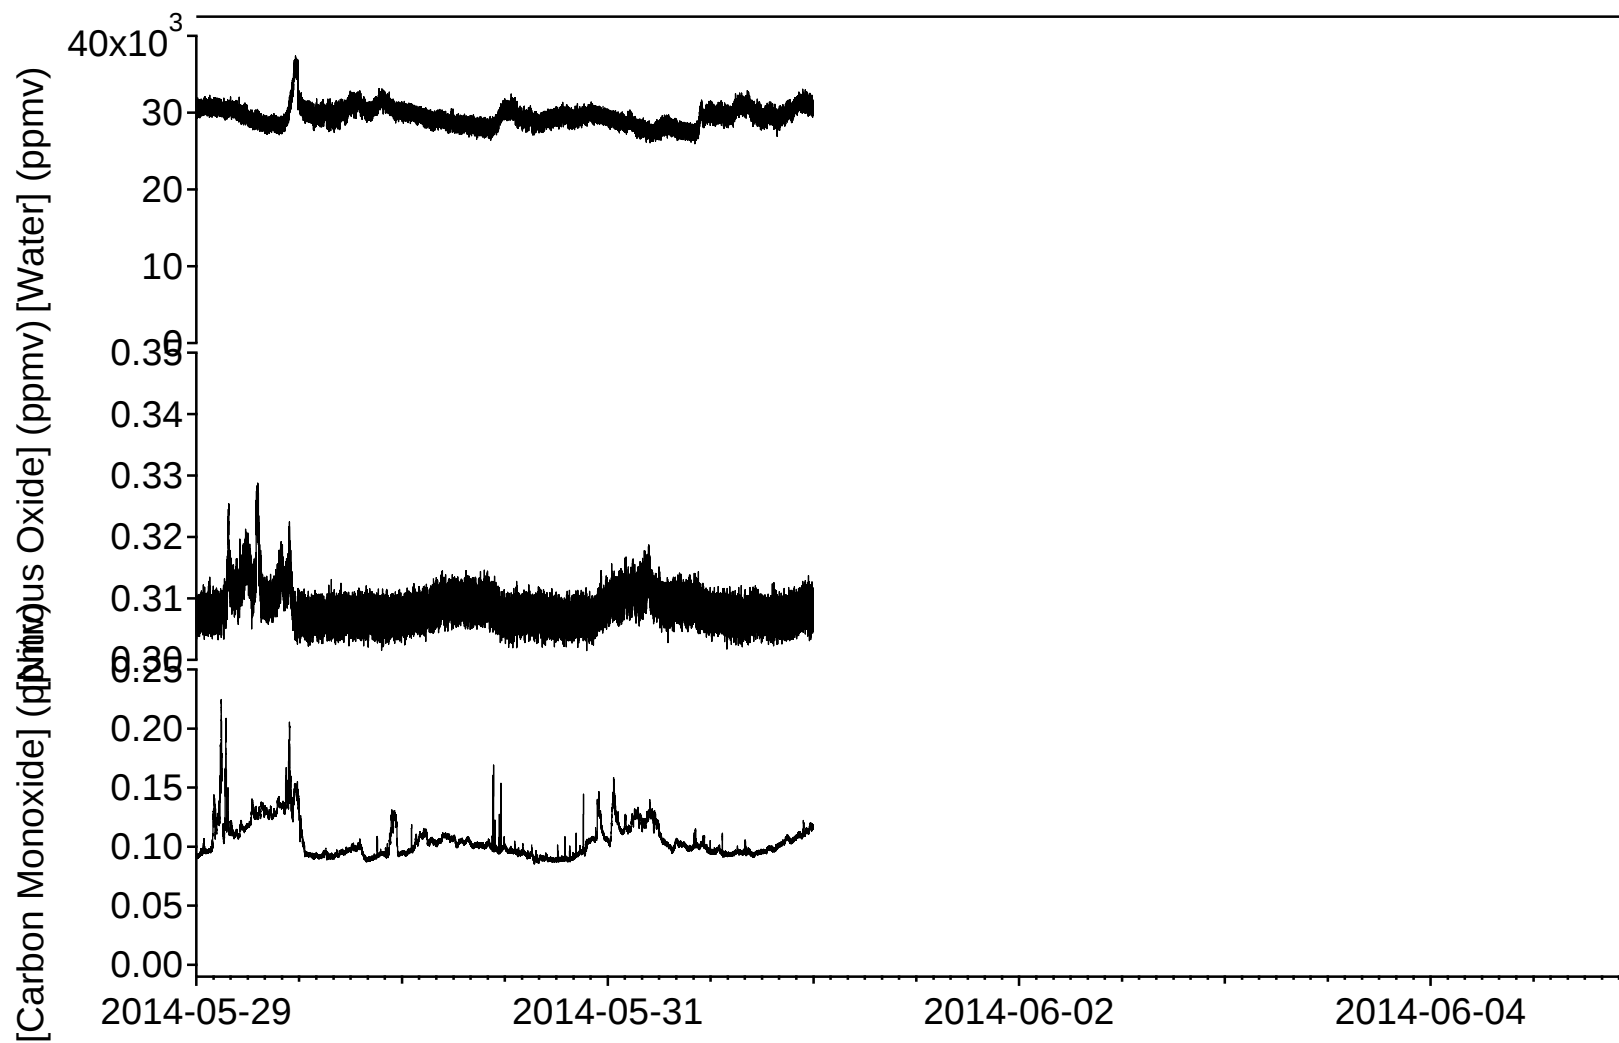

(UTC)

Project/Platform/Site: maomaoscs1
ARM Climate Research Facility
Contact: S.R. Springston (631) 344-4477, srs@bnl.gov