


Processing Record for this file:
(Make notes here unique for this file)

Loading from flight 140925a
Data taken from NOx CPU c:\data\CO


Flight used Dubey Manvendra's mixed gas 'standard'. The actual values of this standard have not yet been provided. On 140912, standard addition frequency changed from 1/30 min to 1/60 min. The CO₂ instrument rebooted in flight. The resulting two data files were concatenated manually. One glitch at beginning of second turn on of CO₂ affected a S.A. This was edited from the data set. Torrential rains during flight. Effects unknown.

Ambient data appear valid.

Los Gatos ICOS CO/N2O/H2O Analyzer
Housekeeping

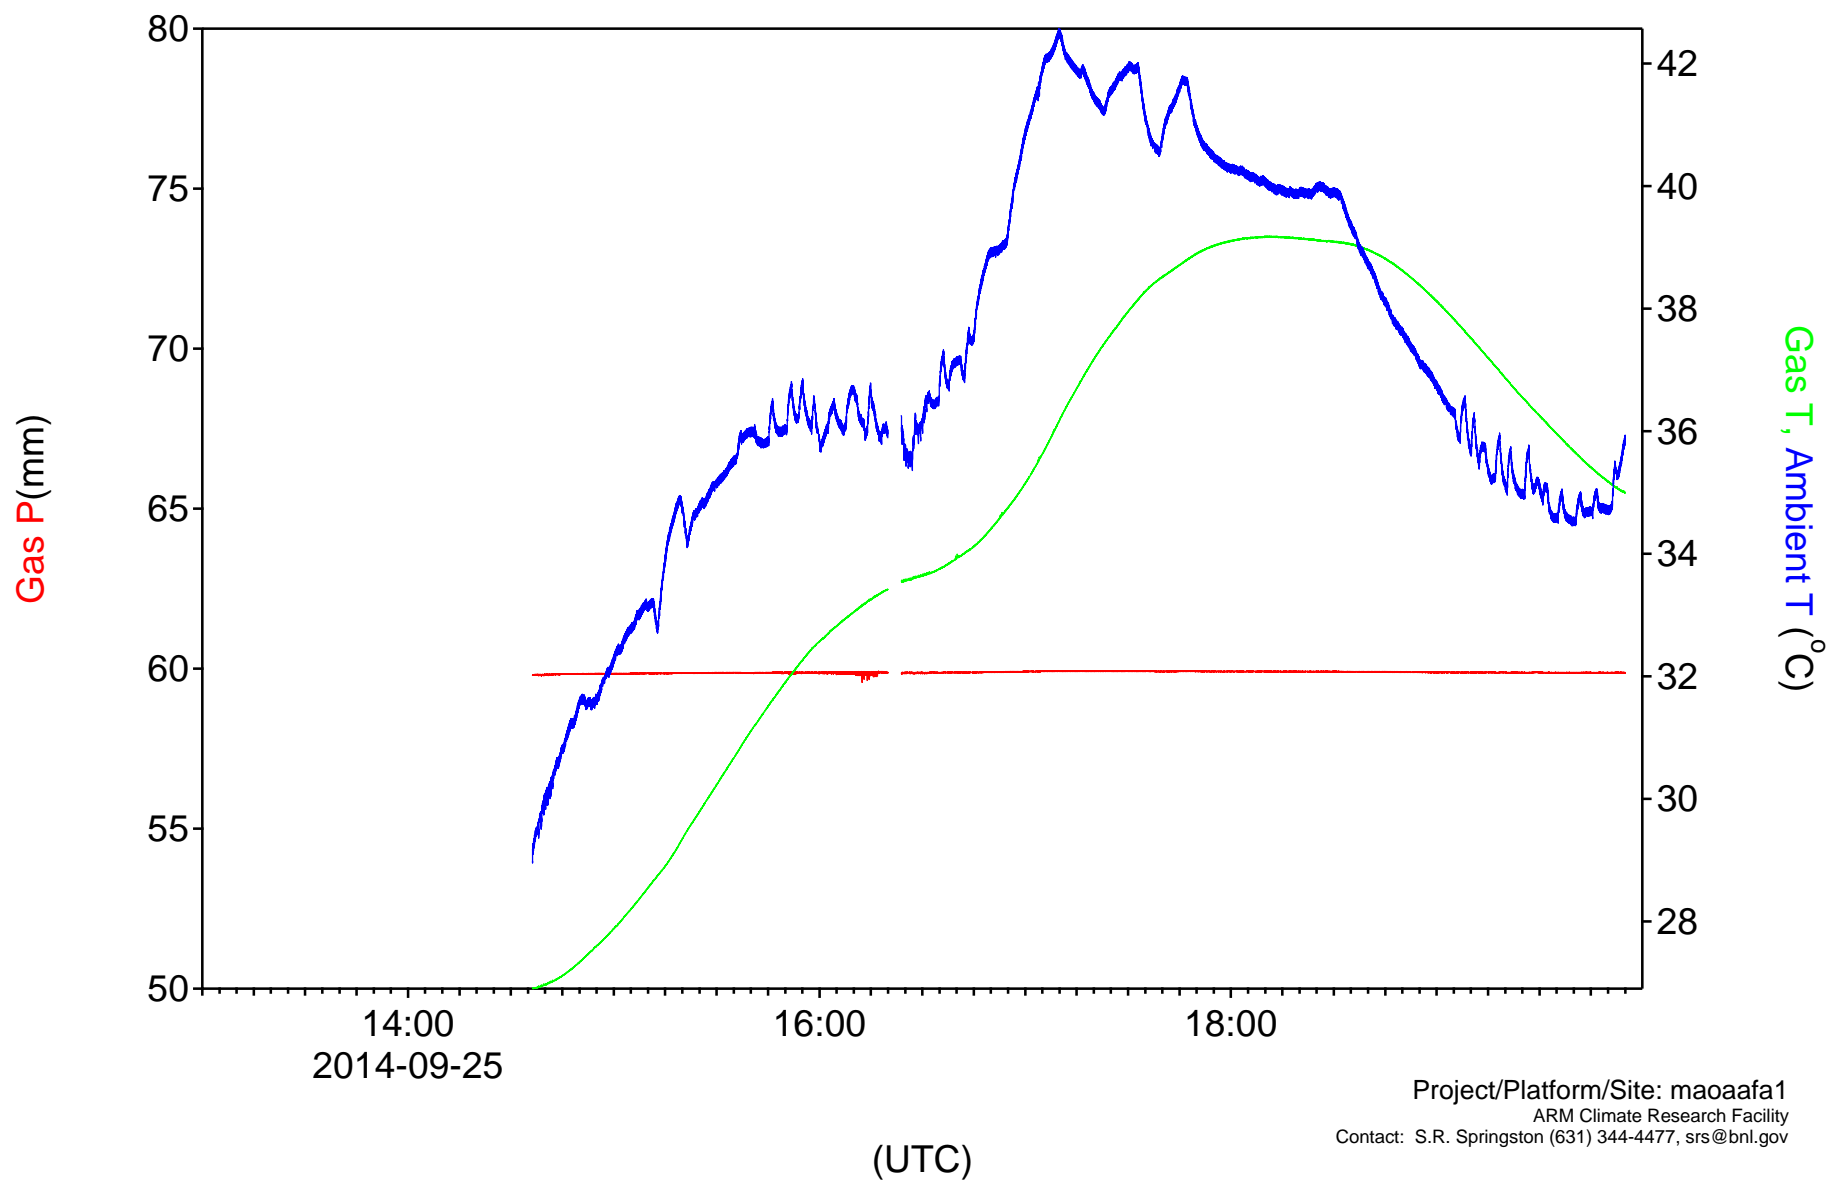

Los Gatos ICOS CO/N₂O/H₂O Analyzer
Data

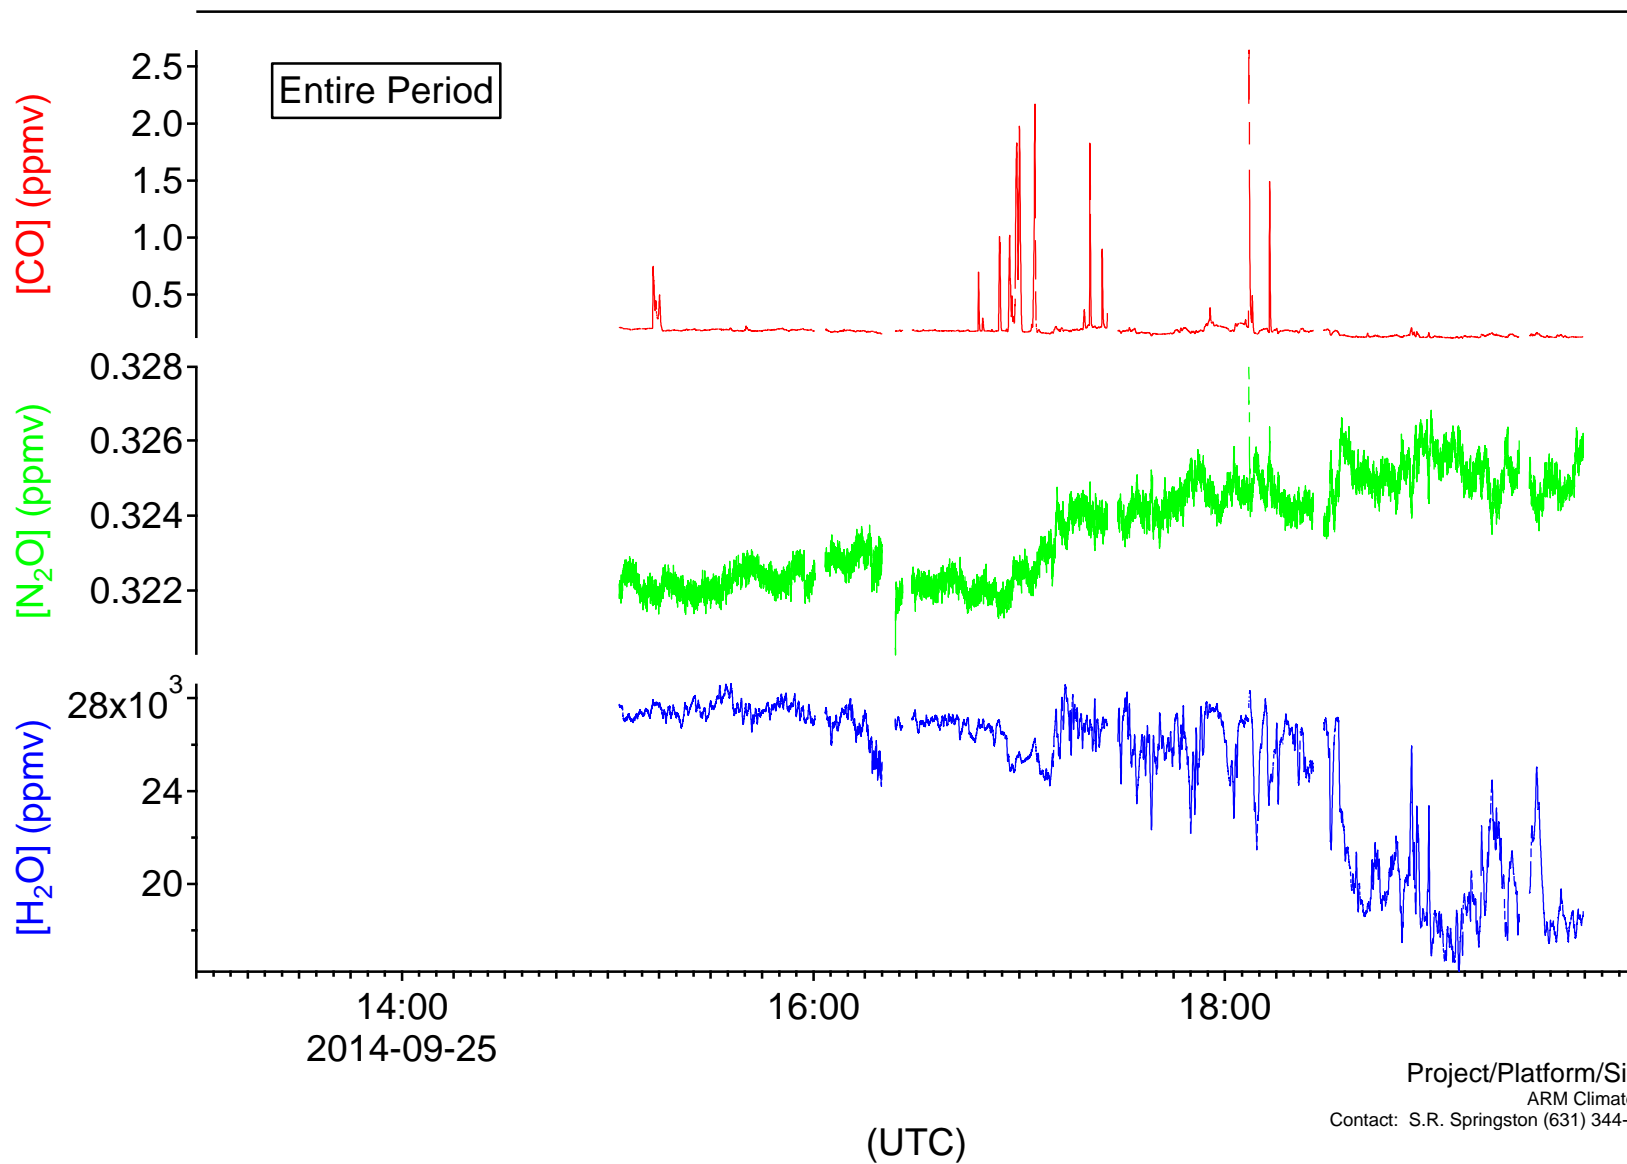

Project/Platform/Site: maoaafa1
ARM Climate Research Facility
Contact: S.R. Springston (631) 344-4477, srs@bnl.gov

Los Gatos ICOS CO/N2O/H2O Analyzer
Raw Data

